

bKIT *Vitis vinifera*

Real-Time PCR assay

Hyris Ltd

HYRIS Headquarters
Lower Ground Floor, One George Yard,
EC3V 9DF, London, UK
Phone: +44.2036082968
Mail: office@hyris.net

HYRIS Research Center
Corso Garibaldi 60,
Milano 20121, Italy
Phone: +39.02.82951302
Mail: administrator@hyris.net

HYRIS Asia Pac
Block 998 Toa Payoh North #06-06
Toa Payoh North Industrial Estate
Singapore 318993, Singapore
Phone: +65.8160.7207
Mail: office@hyris.net

www.hyris.net



Hyris Ltd

HYRIS Headquarters

Lower Ground Floor, One George Yard,
 EC3V 9DF, London, UK
 Phone: +44.2036082968
 Mail: office@hyris.net

HYRIS Research Center

Corso Garibaldi 60,
 Milano 20121, Italy
 Phone: +39.02.82951302
 Mail: administrator@hyris.net

HYRIS Asia Pac

Block 998 Toa Payoh North #06-06
 Toa Payoh North Industrial Estate
 Singapore 318993, Singapore
 Phone: +65.8160.7207
 Mail: office@hyris.net

www.hyris.net

WARNING AND PRECAUTIONS

Do not mix the components of kits with different batch number. This kit is designed to be used by personnel trained to follow correct molecular biology precautions.

WARRANTY AND RESPONSIBILITIES

Hyris Ltd guarantees the buyer exclusively concerning the quality of reagents and of the components used to produce the Kits. Hyris Ltd is not responsible and cannot anyway be considered responsible or jointly responsible for possible direct and indirect damages resulting from the utilization of the Kits by the user. The user consciously and under his/her own responsibilities decides for the utilization purposes of the Kits and uses it the way he/she considers most suitable in order to reach his/her goals and/or objectives.

Hyris is not responsible for the data resulting from the use of the Kits, for the utilization that the user independently decides to make of them or for the direct or indirect damages possibly resulting from the disclosure or transmission of the data themselves to third parties under any form or circumstance. This clause is automatically accepted by the user when purchasing the Kits.

The patent for performing PCR and Real-Time PCR is held by Hoffmann-La Roche. Authorization to use PCR and Real-Time PCR can be obtained on licence from Hoffmann-La Roche. The product, equipment and information included in the Kits consist of assembled reagents. The licence and authorisation for PCR and Real-Time PCR use are not included in the Kits. The user is responsible for setting prefixed goals, choosing whether or not to perform the PCR or Real-Time PCR reaction and to apply for register his/her own licence. The patent for performing LAMP is held by Eiken, from which authorization to use LAMP can be obtained. The licence for LAMP is not included in the Kits.

The Kits are designed for the services supply. Diagnostic applications that are not research use only require a specific licence for PCR and Real-Time PCR or for LAMP use. The Kits may require the use of Taq Polymerase enzyme and/or fluorochromes, often registered as trademark by companies. TaqMan® is a trademark of Roche Molecular Systems, Inc. FAM, VIC and ROX are a trademark of Applied Biosystems Corporation or its affiliate. Cy5 is a trademark of Amersham Biosciences Ltd.

The Kits have been internally tested by our quality control. Any responsibility is waived if the warranty of quality control does not refer to the specific Kits. The user is personally responsible for data that he/she will obtain and/or he/she will supply to third parties using these kits. Once the sealed package is opened the user accepts all the conditions without fail; if the package is still sealed the kit can be returned and the user can be refunded. The Kits are intended for Research Use Only.

Vitis vinifera

Vitis vinifera is one of the most economical important plant species, since it has been extensively used since ancient times for fruits, juice and wine production. *Vitis vinifera* fruit (grape) is also known to contains many bioactive compounds, which have been intensively studied for their antioxidant, anticancer, antibacterial and antidiabetic activities, as well as cardioprotective, hepatoprotective and neuroprotective effects ⁽¹⁾.

⁽¹⁾: Nassiri-Asl M, Hosseinzadeh H. Review of the Pharmacological Effects of *Vitis vinifera* (Grape) and its Bioactive Constituents: An Update. *Phytother Res.* 2016 Sep;30(9):1392-403. doi: 10.1002/ptr.5644. Epub 2016 May 16. Review. PubMed PMID:27196869.

Principle

Hydrolysis probe Real-Time PCR assay for the detection of *Vitis vinifera*. The product is intended for research purpose only.

NHPRA validation

In the validation trials performed by NHPRA (Natural Health Product Research Alliance) the following species were tested: *Acer negundo*, *Ampelopsis brevipedunculata*, *Curcuma longa*, *Echinocystis lobate*, *Panax quinquefolius*, *Parthenocissus quinquefolia*, *Silybum marianum*, *Vitis berlandieri* x *Vitis riparia* and *Vitis riparia*.

bKIT *Vitis vinifera* packaging

Part Number: bKTB-VV.02-50

| | |
|---------------------------|----------|
| qPCR Master Mix (1 tube) | 50 tests |
| Positive Control (1 tube) | 10 tests |
| Negative Control (1 tube) | 10 tests |

Part Number: bKTB-VV.02-100

| | |
|---------------------------|--------------|
| qPCR Master Mix (2 tubes) | 2 x 50 tests |
| Positive Control (1 tube) | 20 tests |
| Negative Control (1 tube) | 20 tests |

Storage

-20°C. Avoid prolonged exposure to light and repeated freeze and thaw cycles.

Shelf life

If the bKIT is correctly stored, at constant-temperature freezer, its performance is guaranteed until the shelf life indicated on the tubes.

Additional material/reagents required

- DNA extraction tools and reagents
- Nuclease-free water
- Gloves
- Pipettes
- bCUBE® instrument or other Real-Time PCR instrument (*) with filters calibrated for FAM
- bCUBE® sample loading cartridge or, if using other Real-Time PCR instrument, samples loading support according to the instrument specifications.

(*) *This assay was especially developed to be used in association with the bCUBE® instrument, available from Hyris Ltd, but can be used also with any other compatible thermal cycler.*

Hyris Ltd

HYRIS Headquarters

Lower Ground Floor, One George Yard,
 EC3V 9DF, London, UK
 Phone: +44.2036082968
 Mail: office@hyris.net

HYRIS Research Center

Corso Garibaldi 60,
 Milano 20121, Italy
 Phone: +39.02.82951302
 Mail: administrator@hyris.net

HYRIS Asia Pac

Block 998 Toa Payoh North #06-06
 Toa Payoh North Industrial Estate
 Singapore 318993, Singapore
 Phone: +65.8160.7207
 Mail: office@hyris.net

www.hyris.net

WARNING AND PRECAUTIONS

Do not mix the components of kits with different batch number. This kit is designed to be used by personnel trained to follow correct molecular biology precautions.

WARRANTY AND RESPONSIBILITIES

Hyris Ltd guarantees the buyer exclusively concerning the quality of reagents and of the components used to produce the Kits. Hyris Ltd is not responsible and cannot anyway be considered responsible or jointly responsible for possible direct and indirect damages resulting from the utilization of the Kits by the user. The user consciously and under his/her own responsibilities decides for the utilization purposes of the Kits and uses it the way he/she considers most suitable in order to reach his/her goals and/or objectives.

Hyris is not responsible for the data resulting from the use of the Kits, for the utilization that the user independently decides to make of them or for the direct or indirect damages possibly resulting from the disclosure or transmission of the data themselves to third parties under any form or circumstance. This clause is automatically accepted by the user when purchasing the Kits.

The patent for performing PCR and Real-Time PCR is held by Hoffmann-La Roche. Authorization to use PCR and Real-Time PCR can be obtained on licence from Hoffmann-La Roche. The product, equipment and information included in the Kits consist of assembled reagents. The licence and authorisation for PCR and Real-Time PCR use are not included in the Kits. The user is responsible for setting prefixed goals, choosing whether or not to perform the PCR or Real-Time PCR reaction and to apply for register his/her own licence. The patent for performing LAMP is held by Eiken, from which authorization to use LAMP can be obtained. The licence for LAMP is not included in the Kits.

The Kits are designed for the services supply. Diagnostic applications that are not research use only require a specific licence for PCR and Real-Time PCR or for LAMP use. The Kits may require the use of Taq Polymerase enzyme and/or fluorochromes, often registered as trademark by companies. TaqMan® is a trademark of Roche Molecular Systems, Inc. FAM, VIC and ROX are a trademark of Applied Biosystems Corporation or its affiliate. Cy5 is a trademark of Amersham Biosciences Ltd.

The Kits have been internally tested by our quality control. Any responsibility is waived if the warranty of quality control does not refer to the specific Kits. The user is personally responsible for data that he/she will obtain and/or he/she will supply to third parties using these kits. Once the sealed package is opened the user accepts all the conditions without fail; if the package is still sealed the kit can be returned and the user can be refunded. The Kits are intended for Research Use Only.

DNA extraction

Extract DNA from samples according to your usual protocol. If necessary, Hyris can recommend an extraction method. At this purpose, contact us at support@hyris.net.

Reaction Set-Up

- Thaw all the bKIT components by placing the tubes on ice.
- Gently mix the tubes content by swirling the tubes.
- Spin the tubes to let the content down.
- In new tubes, one for each sample, including the **Negative Control** and the **Positive Control** of the bKIT, prepare the Reaction Mix as shown in the table below:

| Components | Volume |
|--|---------|
| DNA sample or Positive Control or Negative Control | 3,5 µl |
| qPCR Mastermix | 16,5 µl |
| Total Volume | 20 µl |

Cartridge set-up

The procedure described is for the bCUBE® cartridge, but, if using a different Real-Time PCR instrument, the same procedure can be adopted for other loading sample supports with minor modifications.

1. Samples set-up

The procedure described is for the bCUBE® cartridge, but, if using a different Real-Time PCR instrument, the same procedure can be adopted for other loading sample supports with minor modifications.

- Samples of the following types must be prepared to be loaded on the cartridge:
Positive Control for *Vitis vinifera*
Negative Control for *Vitis vinifera*
 Sample(s) to be tested.

2. Cartridge Loading

- Load the sample prepared as described in the previous section
- Carefully seal the cartridge with adhesive film in order to avoid any contamination.
- Load the cartridge onto the bCUBE®, then start the run.

Method set-up

Set up the run method using the following conditions, depending on the instrument you use.

1. On the bCUBE®

- Login on the bAPP.
- Set-up “New Analysis” and Select the “*Vitis vinifera* 1.x” from the Global Recipes on the bAPP.
- Define your wells types as follows (**Fig. 1**):
 “PosCtrl” for the well loaded with *Vitis vinifera* **Positive Control**.
 “NegCtrl” for the well loaded with *Vitis vinifera* **Negative Control**.
 “Sample” for the wells loaded with samples under analysis.

Hyris Ltd

HYRIS Headquarters
 Lower Ground Floor, One George Yard,
 EC3V 9DF, London, UK
 Phone: +44.2036082968
 Mail: office@hyris.net

HYRIS Research Center
 Corso Garibaldi 60,
 Milano 20121, Italy
 Phone: +39.02.82951302
 Mail: administrator@hyris.net

HYRIS Asia Pac
 Block 998 Toa Payoh North #06-06
 Toa Payoh North Industrial Estate
 Singapore 318993, Singapore
 Phone: +65.8160.7207
 Mail: office@hyris.net

www.hyris.net

WARNING AND PRECAUTIONS

Do not mix the components of kits with different batch number. This kit is designed to be used by personnel trained to follow correct molecular biology precautions.

WARRANTY AND RESPONSIBILITIES

Hyris Ltd guarantees the buyer exclusively concerning the quality of reagents and of the components used to produce the Kits. Hyris Ltd is not responsible and cannot anyway be considered responsible or jointly responsible for possible direct and indirect damages resulting from the utilization of the Kits by the user. The user consciously and under his/her own responsibilities decides for the utilization purposes of the Kits and uses it the way he/she considers most suitable in order to reach his/her goals and/or objectives.

Hyris is not responsible for the data resulting from the use of the Kits, for the utilization that the user independently decides to make of them or for the direct or indirect damages possibly resulting from the disclosure or transmission of the data themselves to third parties under any form or circumstance. This clause is automatically accepted by the user when purchasing the Kits.

The patent for performing PCR and Real-Time PCR is held by Hoffmann/La Roche. Authorization to use PCR and Real-Time PCR can be obtained on licence from Hoffmann-La Roche. The product, equipment and information included in the Kits consist of assembled reagents. The licence and authorisation for PCR and Real-Time PCR use are not included in the Kits. The user is responsible for setting prefixed goals, choosing whether or not to perform the PCR or Real-Time PCR reaction and to apply for register his/her own licence. The patent for performing LAMP is held by Eiken, from which authorization to use LAMP can be obtained. The licence for LAMP is not included in the Kits.

The Kits are designed for the services supply. Diagnostic applications that are not research use only require a specific licence for PCR and Real-Time PCR or for LAMP use. The Kits may require the use of Taq Polymerase enzyme and/or fluorochromes, often registered as trademark by companies. TaqMan® is a trademark of Roche Molecular Systems, Inc. FAM, VIC and ROX are a trademark of Applied Biosystems Corporation or its affiliate. Cy5 is a trademark of Amersham Biosciences Ltd.

The Kits have been internally tested by our quality control. Any responsibility is waived if the warranty of quality control does not refer to the specific Kits. The user is personally responsible for data that he/she will obtain and/or he/she will supply to third parties using these kits. Once the sealed package is opened the user accepts all the conditions without fail; if the package is still sealed the kit can be returned and the user can be refunded. The Kits are intended for Research Use Only.



Fig 1. Cartridge set-up

An example of cartridge set-up on the bAPP for one replicate of a sample to be analyzed is shown.

2. On a compatible Real-Time PCR instrument

Please, contact us for the protocol set-up on the instrument.

Results analysis

1. On the bCUBE®

- a. The presence of the target *Vitis vinifera* in the Positive Control or in the sample under analysis will generate an amplification curve (Fig. 2)

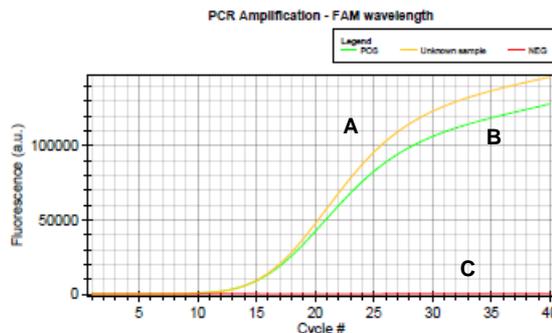


Fig.2. Amplification and melting plots

In the plots, the amplification curve of a *Vitis vinifera* target containing sample (A), a Positive Control (B) and a Negative Control (C) are shown.

- b. At the end of analysis each well will be labelled depending on the well type as described in the tables below:

| Well | Possible labels | |
|----------------------------|-----------------------------|----------------------------|
| Positive Control (PosCtrl) | OK | KO |
| Label meaning | Amplification curve present | Amplification curve absent |

| Well | Possible labels | |
|----------------------------|----------------------------|-----------------------------|
| Negative Control (NegCtrl) | OK | KO |
| Label meaning | Amplification curve absent | Amplification curve present |

| Well | Possible labels | | |
|---------------|--|---|--|
| Sample | Present | Absent | Indeterminate |
| Label meaning | <i>Vitis vinifera</i> is present in the sample | <i>Vitis vinifera</i> is absent from the sample | The test is not conclusive and should be repeated (**) |

(**) If the Indeterminate classification persists, contact us at support@hyris.net

- c. On the bAPP, and on the pdf report of the analysis, the samples classification will be also shown (Fig. 3).

Hyris Ltd

HYRIS Headquarters

Lower Ground Floor, One George Yard,
 EC3V 9DF, London, UK
 Phone: +44.2036082968
 Mail: office@hyris.net

HYRIS Research Center

Corso Garibaldi 60,
 Milano 20121, Italy
 Phone: +39.02.82951302
 Mail: administrator@hyris.net

HYRIS Asia Pac

Block 998 Toa Payoh North #06-06
 Toa Payoh North Industrial Estate
 Singapore 318993, Singapore
 Phone: +65.8160.7207
 Mail: office@hyris.net

www.hyris.net

WARNING AND PRECAUTIONS

Do not mix the components of kits with different batch number. This kit is designed to be used by personnel trained to follow correct molecular biology precautions.

WARRANTY AND RESPONSIBILITIES

Hyris Ltd guarantees the buyer exclusively concerning the quality of reagents and of the components used to produce the Kits. Hyris Ltd is not responsible and cannot anyway be considered responsible or jointly responsible for possible direct and indirect damages resulting from the utilization of the Kits by the user. The user consciously and under his/her own responsibilities decides for the utilization purposes of the Kits and uses it the way he/she considers most suitable in order to reach his/her goals and/or objectives.

Hyris is not responsible for the data resulting from the use of the Kits, for the utilization that the user independently decides to make of them or for the direct or indirect damages possibly resulting from the disclosure or transmission of the data themselves to third parties under any form or circumstance. This clause is automatically accepted by the user when purchasing the Kits.

The patent for performing PCR and Real-Time PCR is held by Hoffmann-La Roche. Authorization to use PCR and Real-Time PCR can be obtained on licence from Hoffmann-La Roche. The product, equipment and information included in the Kits consist of assembled reagents. The licence and authorisation for PCR and Real-Time PCR use are not included in the Kits. The user is responsible for setting prefixed goals, choosing whether or not to perform the PCR or Real-Time PCR reaction and to apply for register his/her own licence. The patent for performing LAMP is held by Eiken, from which authorization to use LAMP can be obtained. The licence for LAMP is not included in the Kits.

The Kits are designed for the services supply. Diagnostic applications that are not research use only require a specific licence for PCR and Real-Time PCR or for LAMP use. The Kits may require the use of Taq Polymerase enzyme and/or fluorochromes, often registered as trademark by companies. TaqMan® is a trademark of Roche Molecular Systems, Inc. FAM, VIC and ROX are a trademark of Applied Biosystems Corporation or its affiliate. Cy5 is a trademark of Amersham Biosciences Ltd.

The Kits have been internally tested by our quality control. Any responsibility is waived if the warranty of quality control does not refer to the specific Kits. The user is personally responsible for data that he/she will obtain and/or he/she will supply to third parties using these kits. Once the sealed package is opened the user accepts all the conditions without fail; if the package is still sealed the kit can be returned and the user can be refunded. The Kits are intended for Research Use Only.

| Results for target <i>Vitis vinifera</i> | |
|--|---------|
| Positive control (PosCtrl) | OK |
| Unknown sample (Sample) | Present |
| Negative control (NegCtrl) | OK |

Fig.3. Analysis results table

The results table, as reported in the pdf report of the analysis, is shown.

2. On a compatible Real-Time PCR instrument

Please, contact us for results interpretation.

Troubleshooting

1. Results show no amplification, or anomalous amplification curves

| Possible causes | Corrective actions |
|---|---|
| Evaporation of the sample due to inadequate sealing of the plate/strips | Repeat the test using the appropriate tools to seal correctly the plate/strips |
| Consumables are not appropriate for the method | Repeat the test using consumables recommended by the supplier of the Real-Time PCR instrument |
| The quality of nucleic acid extracted is low | Repeat the extraction step. Ensure that the method of extraction has been performed correctly. In any doubt, contact us |

2. No amplification curve is observed for the Positive Control

| Possible causes | Corrective actions |
|---|--|
| The Positive Control provided with the assay was not added into the reaction well | Repeat the test. If the problem persists, contact us |

3. An amplification curve is observed for the Negative Control

| Possible causes | Corrective actions |
|---|---|
| Contamination of the Negative Control or the qPCR Master Mix with target-positive DNA | Repeat the test by applying appropriate quality procedures to prevent contamination. If the problem persists, contact us. Correctly seal the cartridge or plate/strips |

Document revision March 01st 2019